



Certificate of Analysis

ILS Laboratories
8222 Vickers St, Suite 106, San Diego, CA 92111
(619) 329-3999 | ils-lab.com

SEMAX - 10mg
Tested for: PureCompoundingLabs.com
www.purecompoundinglabs.com

PASS

COA #: COA-2026-AZ67NR
Lot Number: LOT-2026-332
Accession #: ACC-2026-5962
Labeled Content: 10mg

Analysis Date: 06/30/2026
Appearance: Good
Sample Matrix: Lyophilized
Vial Size: 3mL
Date Received: 06/21/2026



Method: Purity & Quant (HPLC)

Identity
SEMAX


Peptide Purity
99.89%

Fentanyl Free

Purity & Quant (HPLC)

Analyte	Specification	Result	Unit	Status
Peptide Purity (HPLC)	>= 95.0%	99.89%	%	PASS
Net Peptide Content	Report Only	10.41	mg	N/A
Identity (HPLC-RTM)	Semax	Confirmed	-	PASS
Fentanyl Screen	Immunoassay, 50 ng/mL cutoff	Not Detected	-	PASS

HPLC Chromatogram

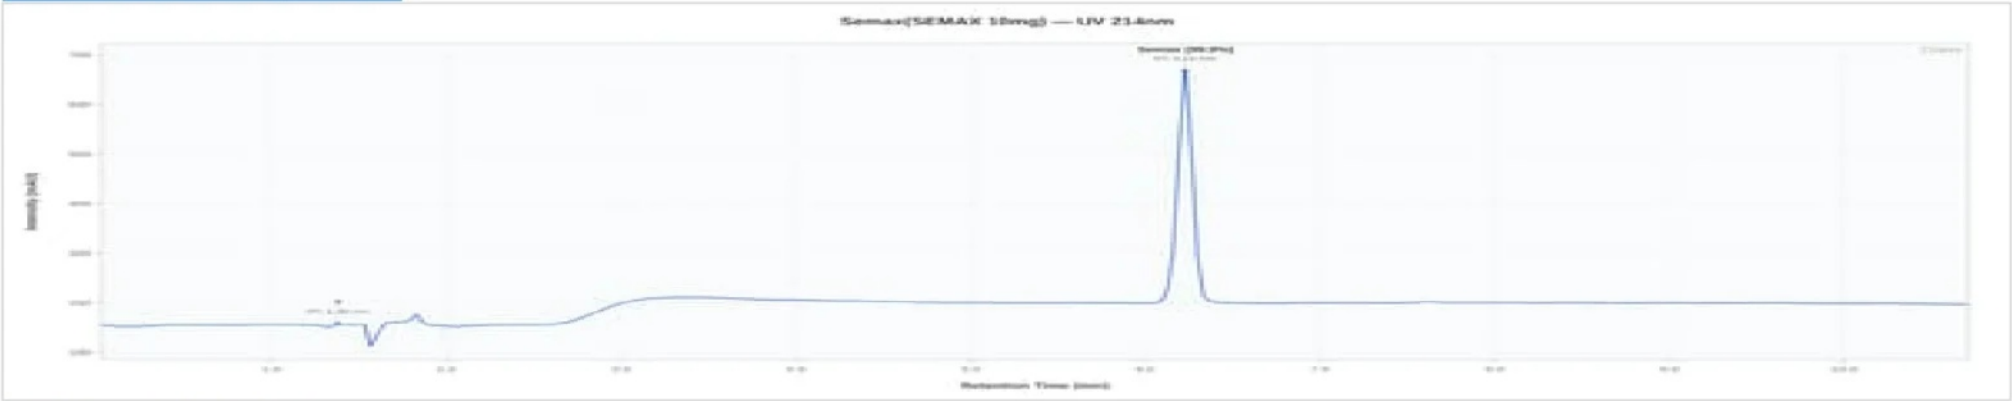

SEMAX 10mg - LOT-2026-332: UV Chromatogram

Notes & Methodology

- 1. Date Tested: 06/30/2026. Methods: Purity & Quant (HPLC).
- 2. The sample was confirmed to be SEMAX by HPLC. Identification by chromatographic retention time comparison with a reference standard.
- 3. Peptide purity determined by RP-HPLC area normalization at 214 nm. Value represents the percentage of the target peptide relative to all peptide-related peaks. Non-peptide process-related impurities, if detected, are excluded from the calculation.



Dr. Greg Kalyuzhny
Lab Director
6/30/2026

COA #: COA-2026-AZ67NR
Access Code: BY6CJKVG
Verify: portal.ils-lab.com/verify/BgkUtYyQHNZq9bUZ
Issued: 6/30/2026